

Sample Received: **March 4, 2026**

COA Issued: **March 6, 2026**

PRODUCT INFORMATION

Vendor: **Upgrade** Sample Name: **5-Amino-1MQ** Sample Type: **Capsule** Batch Number: **70-202602-85**

MW:
159.11 g/mol

ANALYTICAL METHODS


Identity: Confirmed via MALDI-MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS


Specification	Result	Method	Status
Identity: 5-Amino-1MQ	5-Amino-1MQ	MALDI-MS	✓ Conforms
Content	NA mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms

ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 3.058 min)

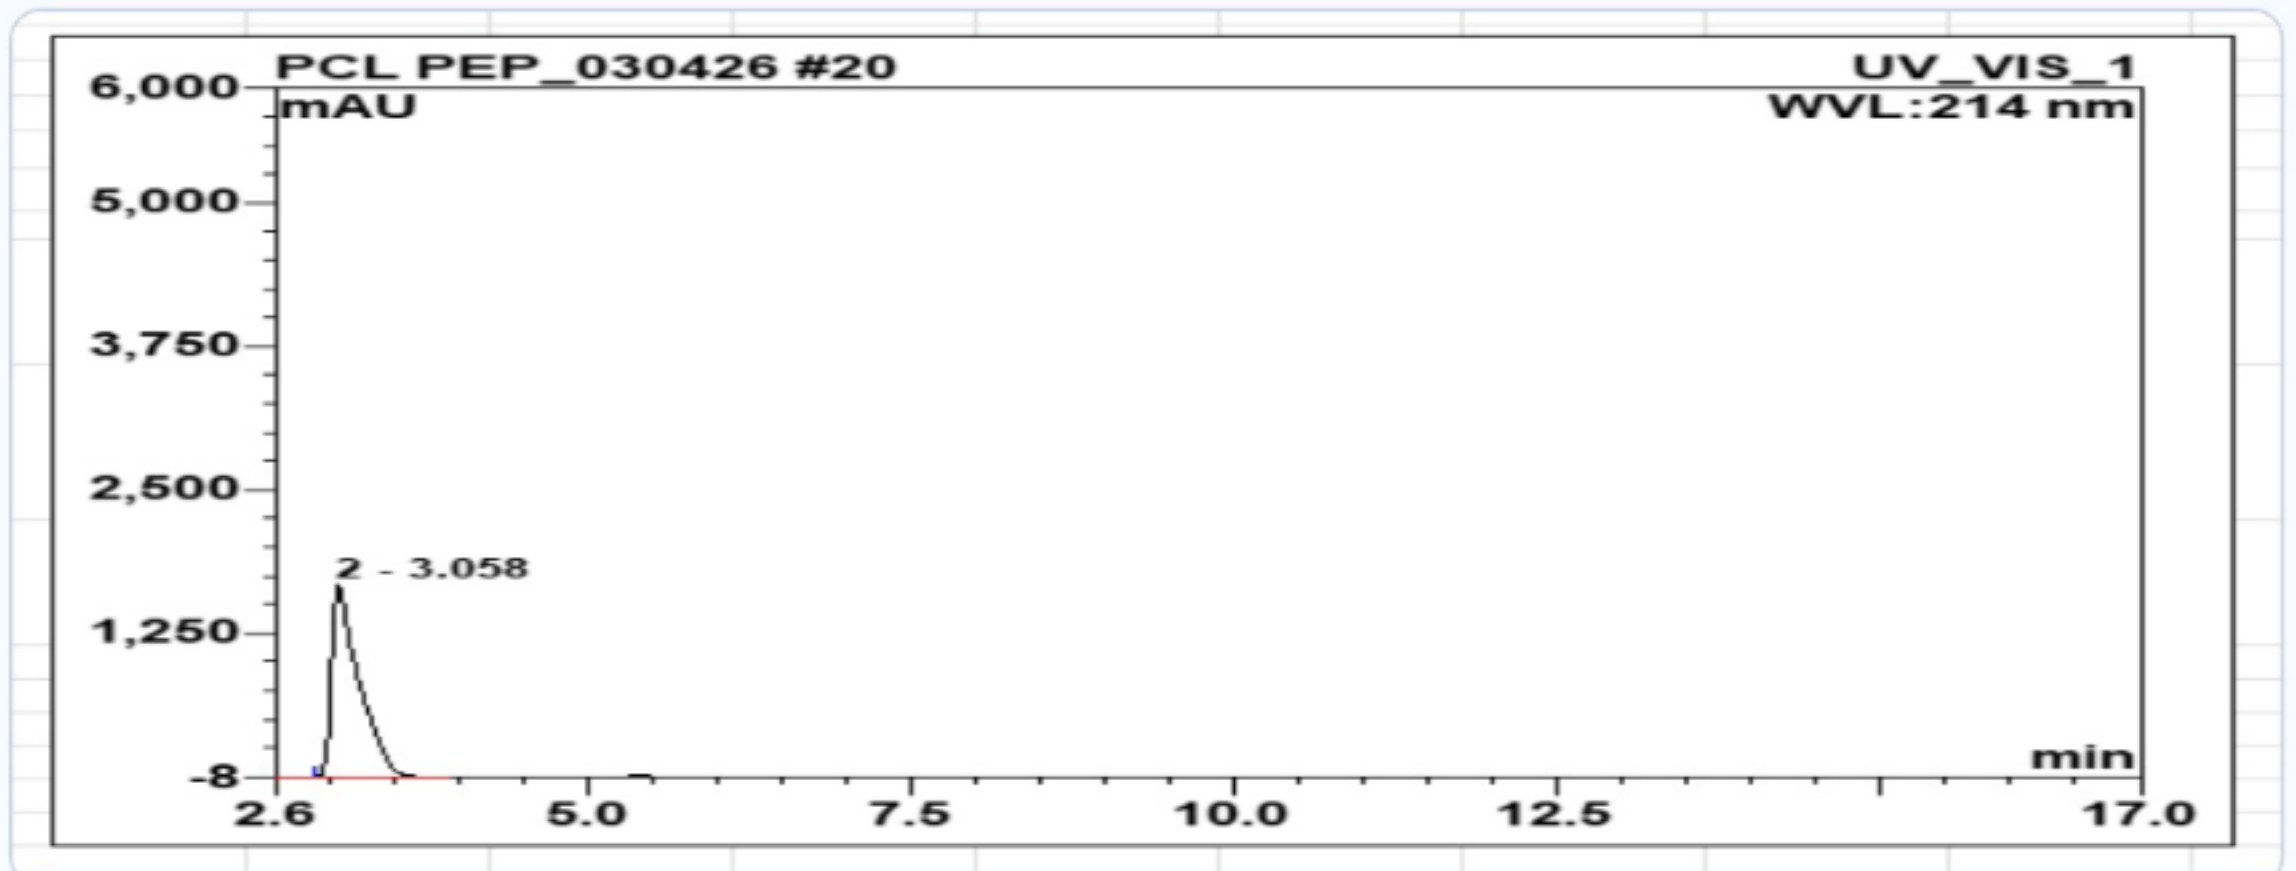

Mass Spectrum (MALDI-MS)

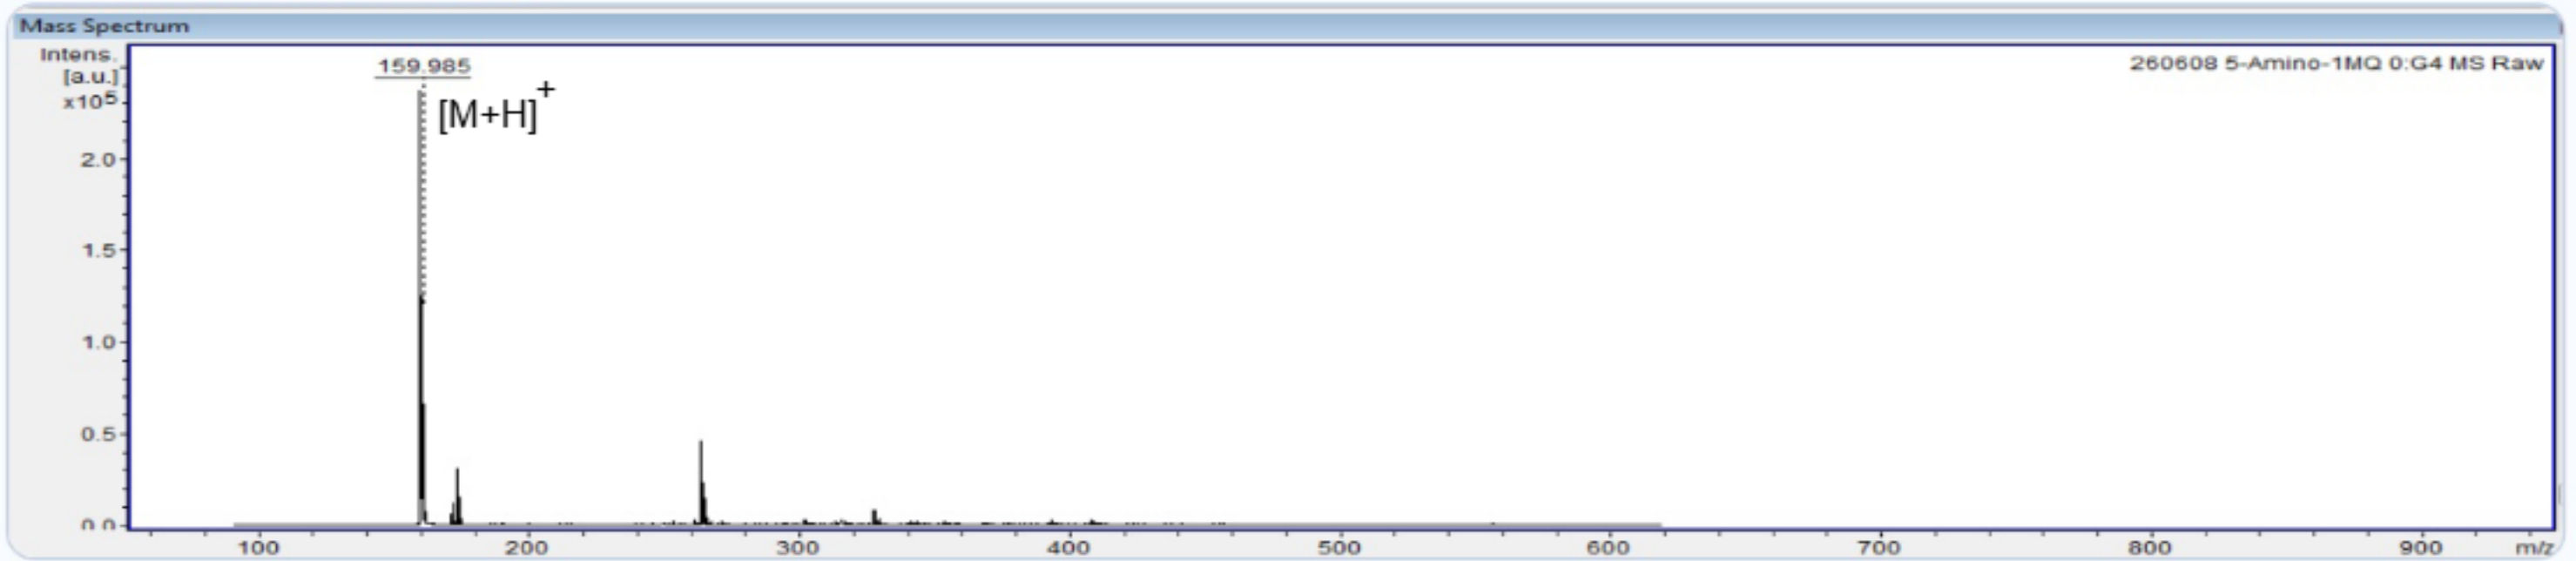

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>



Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.

Contact: info@bioviridians.com