

Sample Received: **February 9, 2026**COA Issued: **February 12, 2026**

PRODUCT INFORMATION

Vendor:
Upgrade WellnessSample Name:
Selank 5mgSample Type:
Nasal sprayBatch Number:
70-202602-73MW:
751.9 g/mol

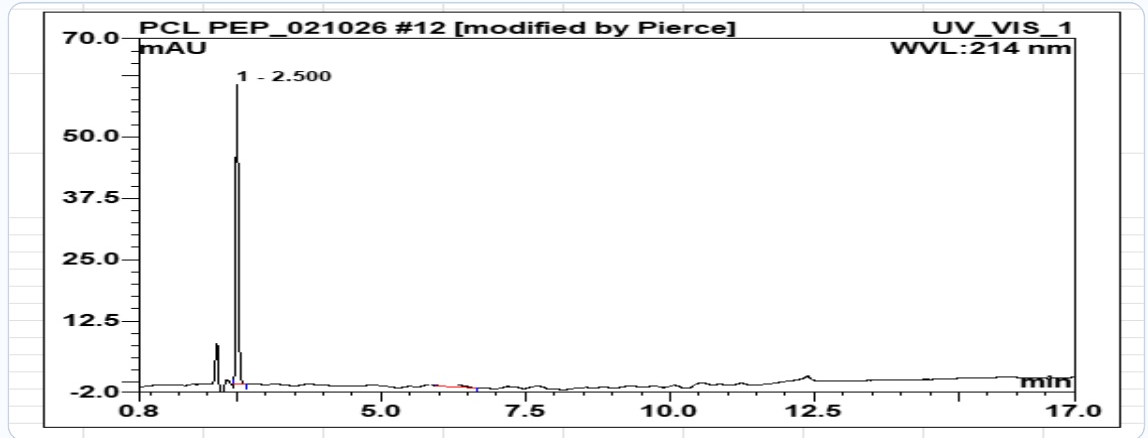
ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS**Purity:** RP-HPLC (214 nm)**Content:** HPLC quantitation

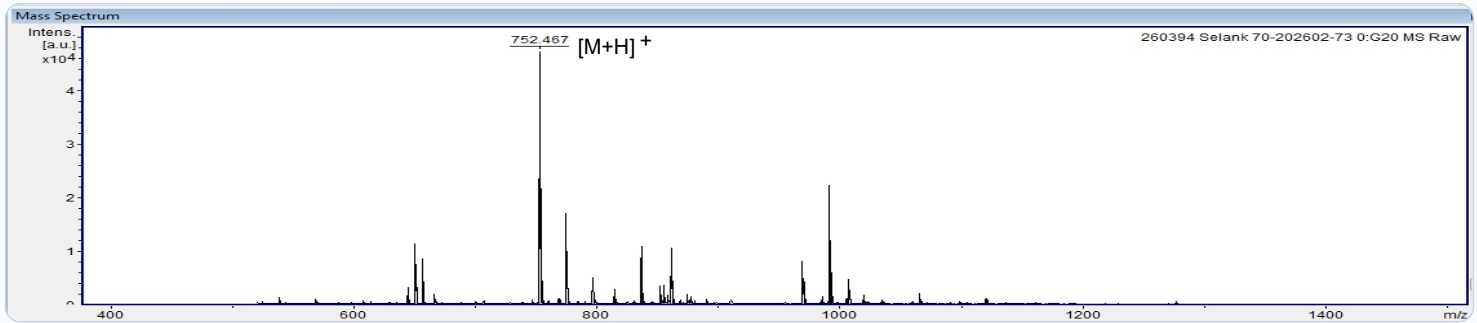
TEST RESULTS

Specification	Result	Method	Status
Identity: Selank	Selank	MALDI-MS	✓ Conforms
Content	5.12 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.6%	RP-HPLC (214 nm)	✓ Conforms

ANALYTICAL DATA

HPLC Chromatogram (Retention Time: 2.500 min)

Mass Spectrum (MALDI-MS)

**Certification:** This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.Visit: <https://bioviridians.com/coa-search.html>*Shane Straight***Shane Straight, M.S.**
Principal Chemist, Bioviridian Inc.Contact: info@bioviridians.com