

Sample Received: **March 4, 2026**

COA Issued: **May 7, 2026**

PRODUCT INFORMATION

Vendor: Upgrade	Sample Name: Semax/Selank 10mg	Sample Type: Nasal spray	Lot Number: NA	MW (g/mol): 813.8, 751.9
---------------------------	--	------------------------------------	--------------------------	------------------------------------

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS



Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Semax with Selank	Semax & Selank	MALDI-MS	✓ Conforms
Content	4.78, 5.23 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.9%	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.525, 6.25 min)

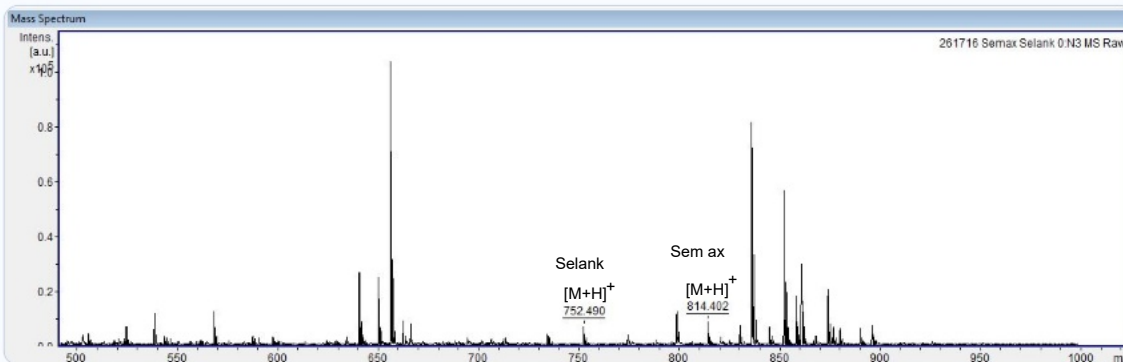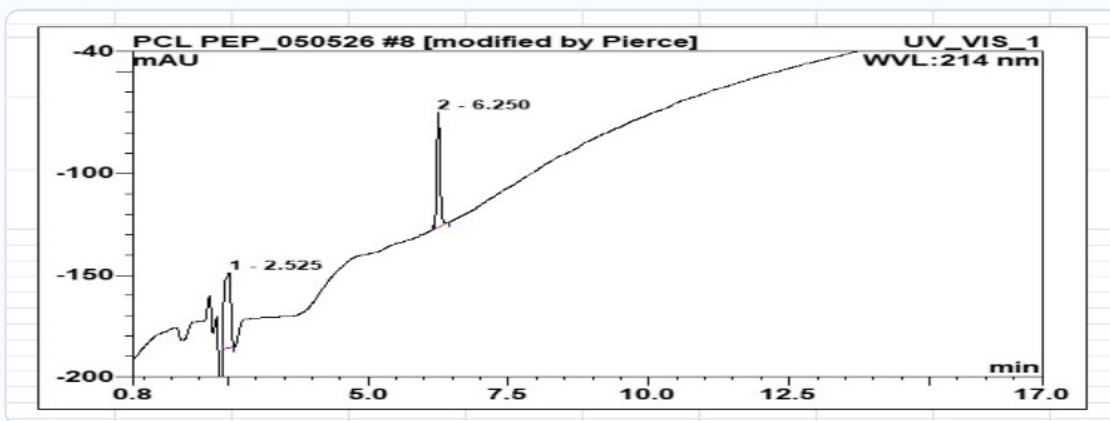

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>



Shane Straight

Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.