

Sample Received: **June 29, 2026**

COA Issued: **July 4, 2026**

PRODUCT INFORMATION

Vendor: **Upgrade** Sample Name: **TRI-BLEND Semax, Selank, D Nasal spray** Sample Type: Lot Number: **80-202606-88** MW (g/mol): **813.9, 751.9, 504.7**

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS




Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: TRI-BLEND Semax, Selank, Dihexa	Semax, Selank, Dihexa	MALDI-MS	✓ Conforms
Content	5.38, 5.69, 5.41 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.300, 9.440, 11.294 min)

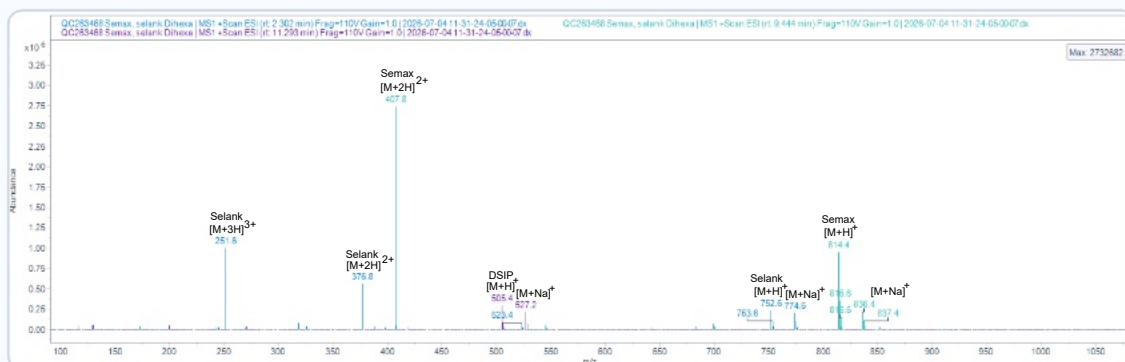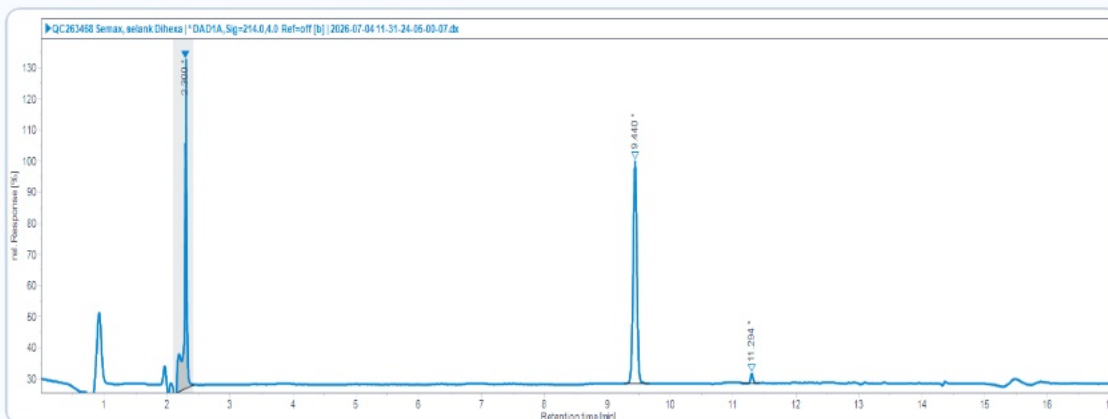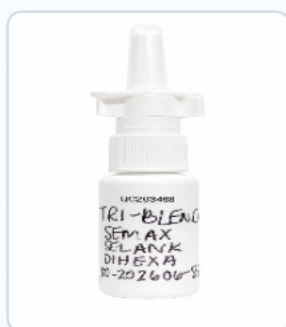

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>



Shane Straight
Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.